


Fiber-Coupled Module

FiCOM B1 λ 930-950 nm

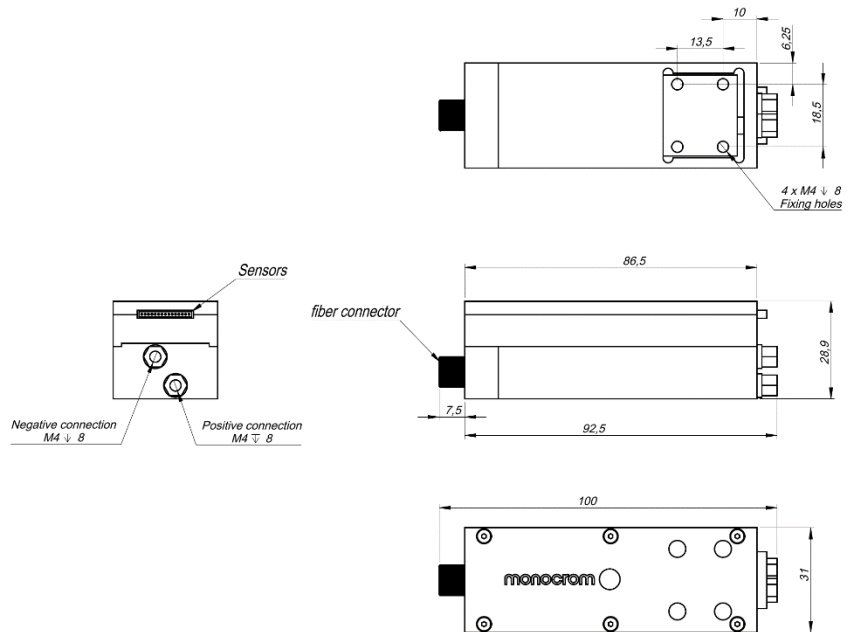

Features:

- Improved cooling efficiency
- No “smile” effect
- No mechanical stress
- Number of bars on demand
- Central wavelength on demand

Suitable for:

- Interstitial laser induced thermotherapy
- Ophthalmology
- Odontology
- Surgical cardiology

- Aesthetics
- Material processing
- Imaging

Technical specifications ^(1,2)	
Wavelength ⁽³⁾ [nm]	930 - 950
Wavelength tolerance [nm]	±5
Spectral width, FWHM [nm]	< 5
Wavelength shift [nm/K]	0.38
Output power ^(2,4) [W]	up to 105
Operating current [A]	< 135
Differential slope, after threshold [W/A]	1.1
Voltage @ connectors ⁽⁵⁾ [V]	2
Fiber core diameter [µm]	down to 200
Numerical aperture	0.22
Fiber input connector	HP-SMA 905
Smile [µm]	< 0.1

1. Specifications at 20 °C, at the beginning of the lifetime
2. Specifications are subject to chips availability
3. Other wavelengths on request
4. Expected output power can varies based on current and temperature
5. Voltage from the power supply must be higher, as due to high current there will be a voltage drop in the cables
6. Pitch dependent

FiCOM B1 / 930 - 950 nm
 Version: 1.0.0.0 October 2021
 Product specifications are subject to change without notice.
 For complete details, please contact your local MONOCROM sales representative.

MONOCROM S.L.
 C/Vilanoveta 6
 08800 Vilanova i la Geltrú
 Spain

T. +34 938 149 450
 E. sales@monocrom.com
www.monocrom.com

UNE EN ISO 9001:2015